
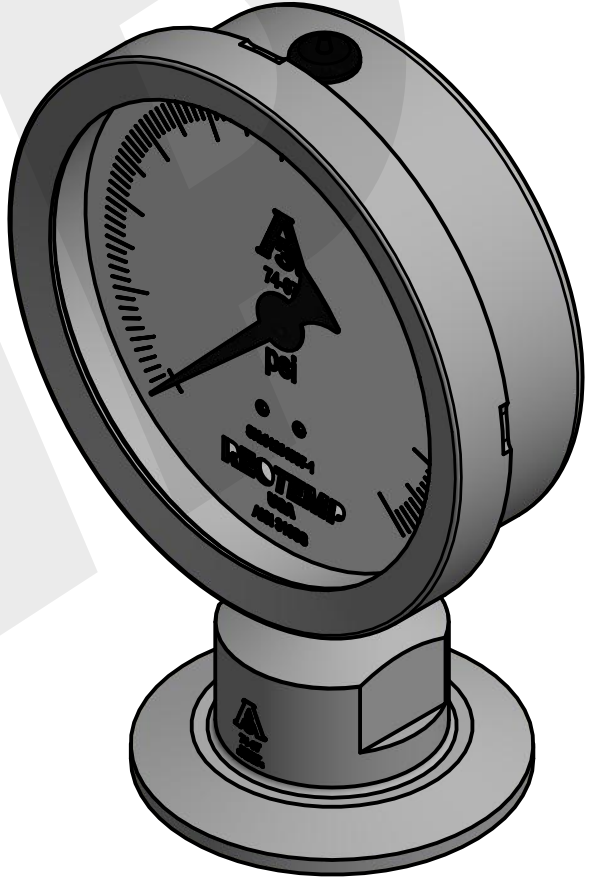


THIS DRAWING AND SPECIFICATIONS ARE THE PROPERTY OF REOTEMP INSTRUMENT CORP., AND ARE ISSUED IN STRICT CONFIDENCE AND SHALL NOT BE REPRODUCED, COPIED OR USED AS THE BASIS FOR MANUFACTURE OR SALE OF ITEMS DEPICTED HEREIN WITHOUT WRITTEN PERMISSION FROM REOTEMP INSTRUMENT CORP.

NOTES (UNLESS OTHERWISE SPECIFIED)

- 1) DIMENSIONS ARE IN INCHES
- 2) PRODUCTS TO BE BUILT PER REOTEMP CATALOG SPECIFICATION, UNLESS OTHERWISE SPECIFIED.

REVISIONS			
REV	DESCRIPTION	DATE	APPROVED
X1	INITIAL	4/28/21	AC

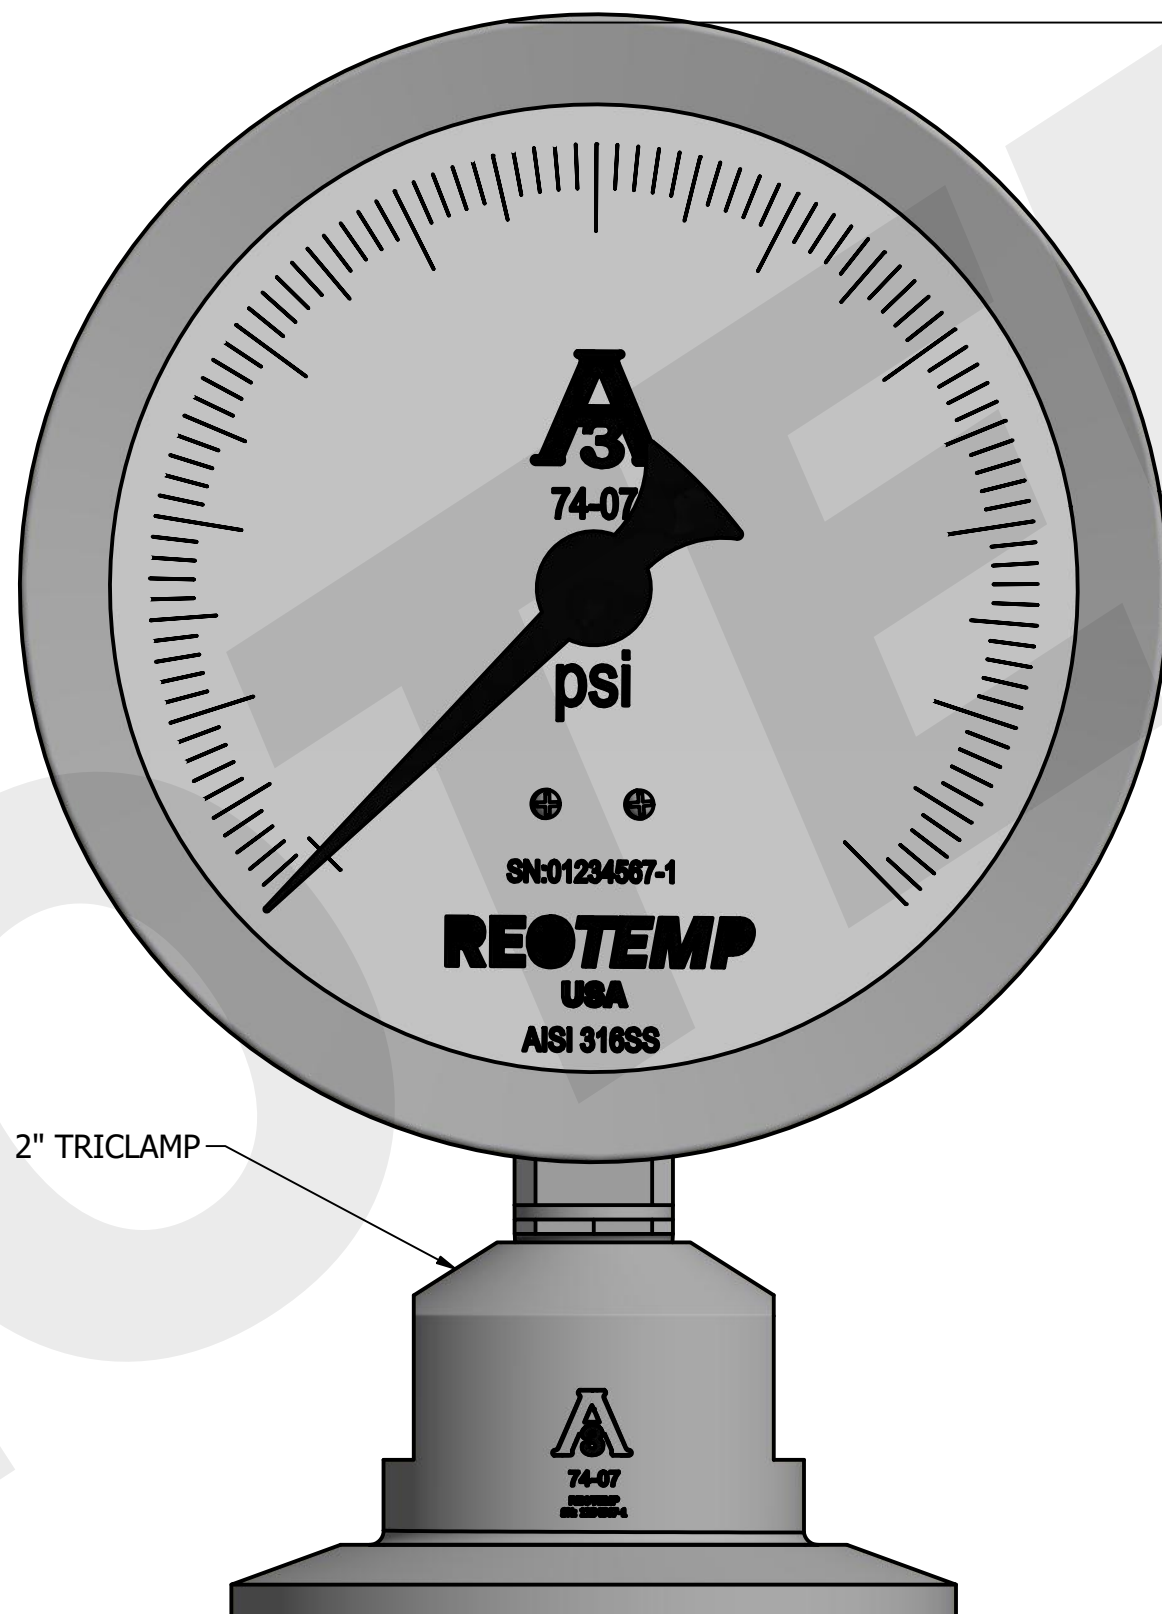

Ø5.5 NOM.

2" TRICLAMP

Ø2.516

PART NAME 3.5" Sanitary Pressure Gauge - Bottom Mount - 2" Triclamp				
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ARE:		Reotemp Instrument Corporation 10656 Roselle Street San Diego, CA 92121 USA Phone: (858) 784-0710 Fax: (858) 784-0720		DATE 4/28/2021
FRACTIONS ±1/32	DECIMALS .X ± .03 .XX ± .01 .XXX ± .005	ANGLES ±1'	REOTEMP	DRAWN BY ACrosby
PART NO SEE PART NAME	SIZE C	CAGE CODE 24793	DWG NO 20892	APPROVED AC
FIRST USED ON	SCALE: NTS	FILE NAME:	REV X1 SHEET 1 OF 1	